

OHSP Test Report

Product Mark


Model: ***UVC
 Temperature: 20°C
 Tester: admin

Manufacture: www.URBI.com.es
 Humidity: 65%
 Test Date: 2020-06-26,11:41:34


Parameter

| Name | Value | Name | Value | Name | Value | Name | Value |
|---------------------------|---------|------------------|-------|------|-------|------|-------|
| ESuv(mW/cm ²) | 0.0324 | Peak Signal | 41431 | | | | |
| Euvc(mW/cm ²) | 0.0164 | Dark Signal | 3917 | | | | |
| Euvb(mW/cm ²) | 0.0271 | Compensate level | 2838 | | | | |
| Euva(mW/cm ²) | 0.0006 | | | | | | |
| Euv(mW/cm ²) | 0.04 | | | | | | |
| Eb(mW/cm ²) | 0.00 | | | | | | |
| Eg(mW/cm ²) | 0.00 | | | | | | |
| Ec(mW/cm ²) | 0.00 | | | | | | |
| Ee(mW/cm ²) | 0.04101 | | | | | | |
| HalfWidth(nm) | 10.3 | | | | | | |
| Peak(nm) | 280.5 | | | | | | |
| Center(nm) | 281.0 | | | | | | |
| Centroid(nm) | 284.1 | | | | | | |
| Integral Time(ms) | 5000.0 | | | | | | |

Spectrogram

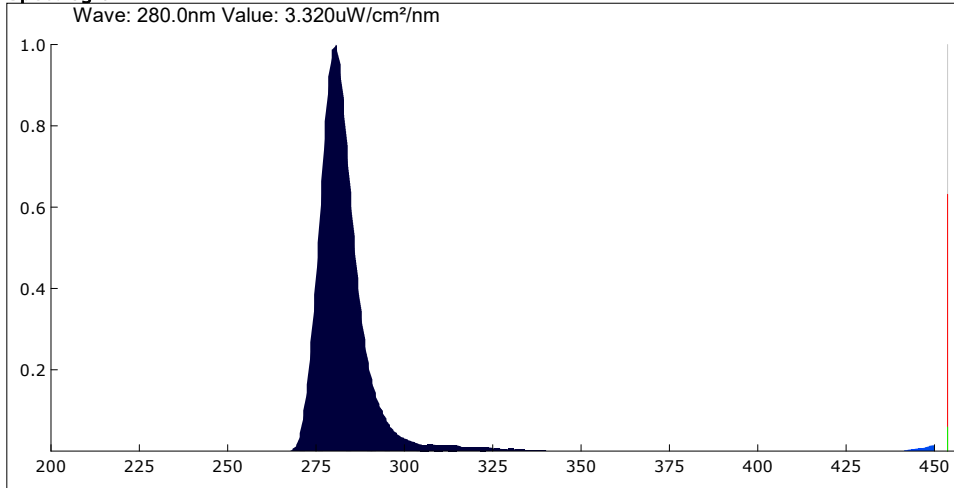


CIE1931



CRI

| | -100 | -75 | -50 | -25 | 0 | 25 | 50 | 75 | 100 |
|-----|------|-----|-----|-----|---|----|----|----|-----|
| Ra | | | | | 0 | | | | |
| R1 | | | | | 0 | | | | |
| R2 | | | | | 0 | | | | |
| R3 | | | | | 0 | | | | |
| R4 | | | | | 0 | | | | |
| R5 | | | | | 0 | | | | |
| R6 | | | | | 0 | | | | |
| R7 | | | | | 0 | | | | |
| R8 | | | | | 0 | | | | |
| R9 | | | | | 0 | | | | |
| R10 | | | | | 0 | | | | |
| R11 | | | | | 0 | | | | |
| R12 | | | | | 0 | | | | |
| R13 | | | | | 0 | | | | |
| R14 | | | | | 0 | | | | |
| R15 | | | | | 0 | | | | |



Instrument Status

Type: OHSP350UVS SN: 0 Scan Range: 200-450nm
 Integral Time: 5000.000ms VPeak: 41431 VDark: 3917